Comfort Inception Cushion - Custom

for ADP in Ontario

Customer information

Date: _____

Company name/ACCT #: _____

Name: _____

Weight: _____

Height: _____

Reference: _____

W/C manufacturer: _____

Model #: _____ Serial #: _____

For best results, do not fill out in your browser. Interactive form should be completed using *Adobe Reader* after saving to your local drive. Then email to sales.ca@permobil.com or print and fax to 877.636.8944.

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

P.O. number: _____

Requested by: _____

Phone: _____ Fax: _____

Email: _____

Ship to: _____

Additional information:

_____

_____

_____

1 Size & shape


1.1 Size

Custom part number:

C-C- W D- -

Please fill in the above with desired dimensions and possible inserts. Example part number for an Inception cushion 15"W x 18"D with a ROHO air insert and ATI: **C-C-15W18D-RI-ATI**

*If desired size is not listed, a 60% upcharge will be applied for materials and Customer Support approval is required.

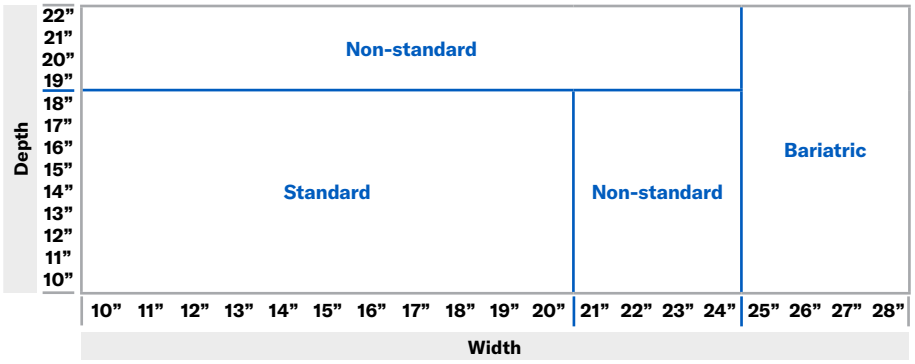


Please note: ADP pricing is listed on page 2 after insert considerations and based on size. Price includes: cushion, inserts, choice of cover, incontinence liner, and HR foam layers.

Seat shape reference guide

Linear


• Base Structure -	Flat Bottom with ¼” Crosslink
• Lower Layer -	1” HR Medium
• Middle Layer -	½” HR Medium
• Topper Layer -	½” Viscool Soft



Anti-thrust

Foam layers as listed in Linear, PLUS...


• Anti-Thrust -	1" H	(15W and above)
½ seat depth	or ½" H	(14W or below)



Zero elevation contour

Foam layers as listed in Linear, PLUS...


• Straight Adductors -	1 ½" H	(15W and above)
	or 1" H	(14W or below)
• Abductor -	1 ½" H	(15W and above)
	or 1" H	(14W or below)



Anti-thrust contour

Foam layers as listed in Linear, PLUS...

• Anti-Thrust -	1" H	(15W and above)
½ seat depth	or ½" H	(14W or below)
• Straight Adductors -	1 ½" H	(15W and above)
	or 1" H	(14W or below)
• Abductor -	1 ½" H	(15W and above)
	or 1" H	(14W or below)



DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

Ischial considerations


There are four ischial modifications available: no insert, Visco foam insert, Gel insert, or ROHO air insert.

If choosing the ROHO air insert, there are specific sizes (min. 16W x 16D), styles, and cutouts required, so please keep these layers and restrictions in mind as you build out the custom Inception (see breakout to right). **The ROHO insert can NOT be paired with:**

- Wedge
- Anti-thrust
- Gel insert or ischial memory foam insert
- Recess
- Coccyx cutout
- Tapered adductors; BUT can be paired with straight adductors if seat is <18"W

Another consideration is the addition of a Moldable ATI (Adjustable Technology Insert for positioning). Please see section 5.10 for details and to select.



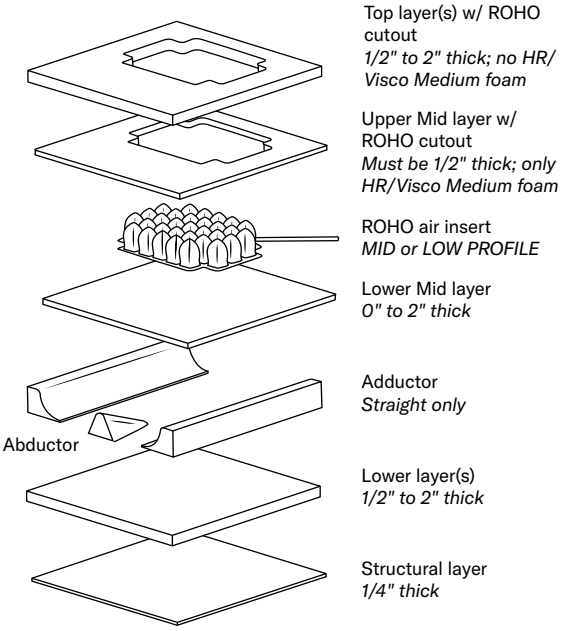


2 Ischial modifications

2.1 Ischial modifications

NOTE: Ischial inserts are recessed into the mid layer of foam and sit beneath the topper layer. **Only one insert may be selected.** Additional ischial modification options on next page.

QuadraGel® insert


NOTE: A minimum of 3/4" mid layer is required for this insert in section 4.3. **Cannot be paired with a ROHO air insert or left/right wedge.**

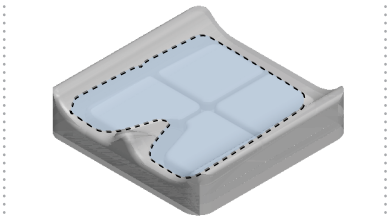

	QuadraGel® insert (CD-QUADRAGEL)

Ischial gel insert


NOTE: A minimum of 1/2" mid layer is required for this insert in section 4.3. **Cannot be paired with a ROHO air insert or left/right wedge.**

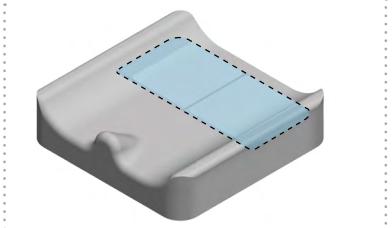

	Ischial gel insert (CD-ISCHIAL-GEL)


Ischial Visco memory foam insert

NOTE: A mid layer of foam must be selected in section 4.3 and, at a minimum, match the insert thickness selected. **Cannot be paired with a ROHO air insert. Foam type cannot match foam type selected for mid layer in 4.3.**

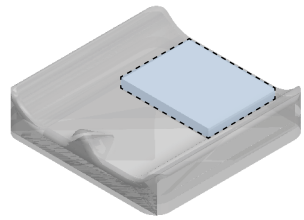

	1" thick soft Visco memory foam insert (CD-ISCHIAL-SOFT-1.0)
	1" thick x-soft Visco memory foam insert (CD-ISCHIAL-XSOFT-1.0)
	1" thick xx-soft Visco memory foam insert (CD-ISCHIAL-XXSOFT-1.0)
	½" thick soft Visco memory foam insert (CD-ISCHIAL-SOFT-0.5)
	½" thick x-soft Visco memory foam insert (CD-ISCHIAL-XSOFT-0.5)
	½" thick xx-soft Visco memory foam insert (CD-ISCHIAL-XXSOFT-0.5)

ROHO® air insert

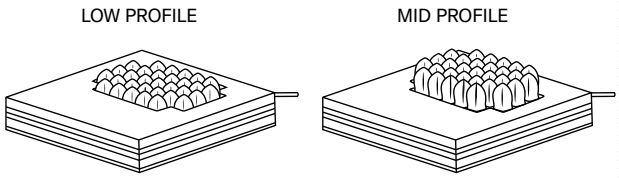

	MID PROFILE® insert (3.25" cell height, 12.5" wide, 9" deep) (CD-ROHO-MID)
	LOW PROFILE® insert (2.25" cell height, 12.5" wide, 9" deep) (CD-ROHO-LOW)

NOTE: ROHO air insert includes hand pump and repair kit. **See above for all the guidelines and restrictions for this ischial insert.**

Pricing (Includes: cushion, inserts, choice of cover, incontinence liner, and HR foam layers)

Cushion size	No ischial insert	Visco foam insert	Gel insert	ROHO insert	No ischial insert, plus ATI	Visco foam insert, plus ATI	Gel insert, plus ATI	ROHO insert, plus ATI
Part number	C-C-__W__D-NI	C-C-__W__D-FI	C-C-__W__D-GI	C-C-__W__D-RI	C-C-__W__D-NI-ATI	C-C-__W__D-FI-ATI	C-C-__W__D-GI-ATI	C-C-__W__D-RI-ATI
Standard	$1,325.00	$1,455.00	$1,515.00	$1,975.00	$1,730.00	$1,860.00	$1,915.00	$2,380.00
Non-Standard >20"W x 18"D	$1,560.00	$1,690.00	$1,750.00	$2,215.00	$1,965.00	$2,095.00	$2,155.00	$2,629.00
Bariatric >24"W	$2,585.00	$2,715.00	$2,770.00	$3,235.00	$2,989.00	$3,115.00	$3,175.00	$3,640.00

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

3 Base specifications

3.1 Bottom style

NOTE: If choosing a wedge in subsection A, proceed to subsection B and choose a wedge height.

A.

NOTE: Only **one** bottom style may be selected. Flat bottom is standard if an alternate style is not selected.

Flat
MSRP $0.00




Front view

	Flat bottom (CD-FLAT-BOTTOM)

NOTE: If a round bottom style is selected, ½" to 1" of additional profile height will be added to the seat support. **Cannot be paired with rigid insert.**

Round
MSRP $57.00





Front view

	Round bottom (CD-ROUND-BOTTOM)

NOTE: A reverse wedge will add height to the rear of the seat support surface. **Cannot be paired with ROHO air insert, only full wedges available with anti-thrust and ischial insert.**

Wedge
MSRP notes in height selection

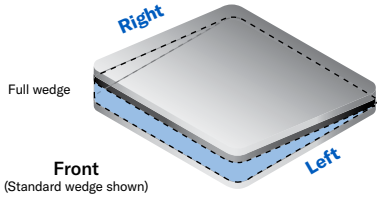

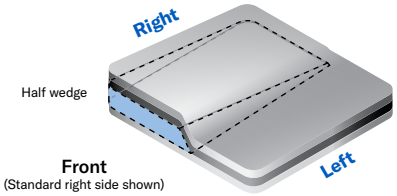


	Standard full wedge (CD-WEDGE-STANDARD)
	Standard left side (CD-WEDGE-LEFT)
	Standard right side (CD-WEDGE-RIGHT)
	Reverse full wedge (CD-WEDGE-REV)
	Reverse left side (CD-WEDGE-REV-LEFT)
	Reverse right side (CD-WEDGE-REV-RIGHT)

B.

NOTE: Wedge is not a removable feature.

Wedge height
MSRP $57.00

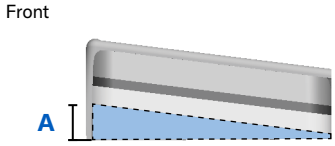


Side view
(Standard style shown)

	A = 1" (CD-WEDGE-1)
	A = 2" (CD-WEDGE-2)
	A = 3" (CD-WEDGE-3)
	A = Other _____ (CD-WEDGE-OTHER)

3.2 Anti-thrust
MSRP $0.00

INSTRUCTIONS: Choose one style and height (directly below your style choice) in subsection A. Anti-thrust will be 1/2 of the seat support depth unless otherwise noted in subsection B. **NOTE**: Depth dimension is determined before growth kit strips are applied. **Cannot be paired with a ROHO air insert or a left or right wedge.**


A. Anti-thrust style & height



Side view

	Standard anti-thrust (CD-AT-STANDARD)
	Left side only (CD-AT-LEFT)
	Right side only (CD-AT-RIGHT)

	B = ½" (CD-AT-HEIGHT-0.5)
	B = 1" (CD-AT-HEIGHT-1.0)
	B = 1 ½" (CD-AT-HEIGHT-1.5)
	B = 2" (CD-AT-HEIGHT-2.0)
	B = 2 ½" (CD-AT-HEIGHT-2.5)
	B = Other _____ (CD-AT-HEIGHT-OTHER)




Side view

	Standard anti-thrust **with growth kit** (CD-AT-STND-GROWTH-KIT)

Anti-Thrust with (3) 1" strips included for growing the Anti-Thrust depth. Top layer foam is not glued in the seat well allowing access to the 1" pieces.

	B = ½" (CD-AT-GK-HEIGHT-0.5)
	B = 1" (CD-AT-GK-HEIGHT-1.0)
	B = 1 ½" (CD-AT-GK-HEIGHT-1.5)
	B = 2" (CD-AT-GK-HEIGHT-2.0)
	B = 2 ½" (CD-AT-GK-HEIGHT-2.5)
	B = Other _____ (CD-AT-GK-HEIGHT-OTHER)

B. Anti-thrust depth

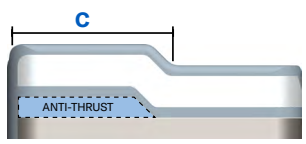

Side view

	C = 4" (CD-AT-DEPTH-4)
	C = 5" (CD-AT-DEPTH-5)
	C = 6" (CD-AT-DEPTH-6)
	C = 7" (CD-AT-DEPTH-7)
	C = 8" (CD-AT-DEPTH-8)
	C = 9" (CD-AT-DEPTH-9)
	C = 10" (CD-AT-DEPTH-10)

	C = 11" (CD-AT-DEPTH-11)
	C = 12" (CD-AT-DEPTH-12)
	C = 13" (CD-AT-DEPTH-13)
	C = 14" (CD-AT-DEPTH-14)
	C = 15" (CD-AT-DEPTH-15)
	C = 16" (CD-AT-DEPTH-16)
	C = Other _____ (CD-AT-DEPTH-OTHER)

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

4 Foam layers

NOTE: If ordering a ROHO air insert, please see page 2 for foam layer restrictions.

Foam recommendations by user weight:

Pediatric or User <100 lb (45 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 1 ½" (lower and mid layer combined)	●	○		○			
Mid layer			○		○	○		
Topper layer	Minimum ¼"			●		○	○	○

Standard user 100 to 350 lb (45-158 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 2 ½" (lower and mid layer combined)	●	○		○			
Mid layer			○		○	○		
Topper layer	Minimum ¼"			●		○	○	○

Bariatric user >350 lb (158 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 3 ½" (lower and mid layer combined)	●	○		○			
Mid layer			○		○			
Topper layer	Minimum ½"		○	●	○	○	○	○


4.1 Structural layer

MSRP $0.00

None CD-FOAM-STRUCTURAL-NONE	
¼" Crosslink CD-FOAM-STRUCTURAL-0.25	

4.2 Lower layers

MSRP HR $0.00 | **Visco** $225.00 each | **Crosslink Firm** $47.00 each




NOTE: We do not recommend a MEDIUM foam on top of a SOFT foam. "Other" Visco foam layer thicknesses must be in 1/2" increments. *Additional foam layers, if chosen, will be placed on top of the original layer.

	Lower layer thickness						*Optional - Additional lower layer thickness					
	**¼"	½"	¾"	1"	1 ¼"	Other 3" Max	¼"	½"	¾"	1"	1 ¼"	OTHER 3" Max
HR Medium	CD-LOW-HRM-0.25	CD-LOW-HRM-0.50	CD-LOW-HRM-0.75	CD-LOW-HRM-1.00	CD-LOW-HRM-1.25	CD-LOW-HRM-OTHER _____	CD-ADD-LOW-HRM-0.25	CD-ADD-LOW-HRM-0.50	CD-ADD-LOW-HRM-0.75	CD-ADD-LOW-HRM-1.00	CD-ADD-LOW-HRM-1.25	CD-ADD-LOW-HRM-OTHER _____
Visco Medium		CD-LOW-VIS-M-0.50		CD-LOW-VIS-M-1.00		CD-ADD-LOW-VIS-M-OTHER _____		CD-ADD-LOW-VIS-M-0.50		CD-ADD-LOW-VIS-M-1.00		CD-ADD-LOW-VIS-M-OTHER _____
Crosslink Firm		CD-LOW-FRM-0.50		CD-LOW-FRM-1.00				CD-ADD-LOW-FRM-0.50		CD-ADD-LOW-FRM-1.00		

**1/4" lower layer is only to be used in conjunction with 1/4" structural layer.

4.3 Mid layers

MSRP HR $0.00 | **Visco** $225.00 each




NOTE: A minimum thickness mid layer must be selected if a QuadraGel insert, ischial gel insert, or ischial memory foam insert is chosen. See section 2.1 for specific details. A recess is cut from the mid layer, so if a recess is selected in section 5.4, the mid layer may need to be thicker to allow for enough support in all areas.

	Mid layer thickness						*Optional - Additional mid layer thickness					
	¼"	½"	¾"	1"	1 ¼"	Other 2" Max	¼"	½"	¾"	1"	1 ¼"	Other 2" Max
HR Medium	CD-MID-HRM-0.25	CD-MID-HRM-0.50	CD-MID-HRM-0.75	CD-MID-HRM-1.00	CD-MID-HRM-1.25	CD-MID-HRM-OTHER _____	CD-Add-Mid-HRM-0.25	CD-Add-Mid-HRM-0.50	CD-Add-Mid-HRM-0.75	CD-Add-Mid-HRM-1.00	CD-Add-Mid-HRM-1.25	CD-Add-Mid-HRM-OTHER _____
HR Soft	CD-MID-HRS-0.25	CD-MID-HRS-0.50	CD-MID-HRS-0.75	CD-MID-HRS-1.00	CD-MID-HRS-1.25	CD-MID-HRS-OTHER _____	CD-Add-Mid-HRS-0.25	CD-Add-Mid-HRS-0.50	CD-Add-Mid-HRS-0.75	CD-Add-Mid-HRS-1.00	CD-Add-Mid-HRS-1.25	CD-Add-Mid-HRS-OTHER _____
Visco Medium		CD-MID-VIS-M-0.50		CD-MID-VIS-M-1.00		CD-MID-VIS-M-OTHER _____		CD-Add-Mid-VIS-M-0.50		CD-Add-Mid-VIS-M-1.00		CD-Add-Mid-VIS-M-OTHER _____
Visco Soft		CD-MID-VIS-S-0.50		CD-MID-VIS-S-1.00		CD-MID-VIS-S-OTHER _____		CD-Add-Mid-VIS-S-0.50		CD-Add-Mid-VIS-S-1.00		CD-Add-Mid-VIS-S-OTHER _____
Visco X-Soft		CD-MID-VIS-XS-0.50		CD-MID-VIS-XS-1.00		CD-MID-VIS-XS-OTHER _____		CD-Add-Mid-VIS-XS-0.50		CD-Add-Mid-VIS-XS-1.00		CD-Add-Mid-VIS-XS-OTHER _____

4.4 Topper layers

MSRP HR $0.00 | **Visco** $225.00 each



NOTE: A minimum 1/4" thick topper layer must be selected here if a QuadraGel insert, ischial gel insert, or ischial memory foam insert was chosen in section 2.1.

	Topper layer thickness						*Optional - Additional topper layer thickness					
	¼"	½"	¾"	1"	1 ¼"	Other 2" Max	¼"	½"	¾"	1"	1 ¼"	Other 2" Max
HR Medium	CD-TOP-HRM-0.25	CD-TOP-HRM-0.50	CD-TOP-HRM-0.75	CD-TOP-HRM-1.00	CD-TOP-HRM-1.25	CD-TOP-HRM-OTHER _____	CD-ADD-TOP-HRM-0.25	CD-ADD-TOP-HRM-0.50	CD-ADD-TOP-HRM-0.75	CD-ADD-TOP-HRM-1.00	CD-ADD-TOP-HRM-1.25	CD-ADD-TOP-HRM-OTHER _____
HR Soft	CD-TOP-HRS-0.25	CD-TOP-HRS-0.50	CD-TOP-HRS-0.75	CD-TOP-HRS-1.00	CD-TOP-HRS-1.25	CD-TOP-HRS-OTHER _____	CD-ADD-TOP-HRS-0.25	CD-ADD-TOP-HRS-0.50	CD-ADD-TOP-HRS-0.75	CD-ADD-TOP-HRS-1.00	CD-ADD-TOP-HRS-1.25	CD-ADD-TOP-HRS-OTHER _____
Visco Medium		CD-TOP-VIS-M-0.50		CD-TOP-VIS-M-1.00		CD-TOP-VIS-M-OTHER _____		CD-ADD-TOP-VIS-M-0.50		CD-ADD-TOP-VIS-M-1.00		CD-ADD-TOP-VIS-M-OTHER _____
Visco Soft		CD-TOP-VIS-S-0.50		CD-TOP-VIS-S-1.00		CD-TOP-VIS-S-OTHER _____		CD-ADD-TOP-VIS-S-0.50		CD-ADD-TOP-VIS-S-1.00		CD-ADD-TOP-VIS-S-OTHER _____
Visco X-Soft		CD-TOP-VIS-XS-0.50		CD-TOP-VIS-XS-1.00		CD-TOP-VIS-XS-OTHER _____		CD-ADD-TOP-VIS-XS-0.50		CD-ADD-TOP-VIS-XS-1.00		CD-ADD-TOP-VIS-XS-OTHER _____
Visco XX-Soft		CD-TOP-VIS-XXS-0.50		CD-TOP-VIS-XXS-1.00		CD-TOP-VIS-XXS-OTHER _____		CD-ADD-TOP-VIS-XXS-0.50		CD-ADD-TOP-VIS-XXS-1.00		CD-ADD-TOP-VIS-XXS-OTHER _____

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

5 Custom specs & geometry

5.1 Adduction


INSTRUCTIONS: Select an adductor height for each side in subsection A, select an adductor style and material for each side in subsection B. If no adduction is needed, choose "none" in subsection A.

If a height is selected but not a style, a full-length, straight, adductor will be applied.

NOTE: Custom adductor requests should be noted in the "Additional information" section 7.1.


NOTE: In subsection B, one adductor style may be selected for each side of the seat support. Front or rear only adductor will be 1/2 the seat support depth or match an anti-thrust depth. **Tapered adductor cannot be paired with ROHO air insert. Straight adductor CAN be paired with a ROHO air insert, but must have a seat width 18" wide or greater.**

FRONT



REAR

Tapered Adductor Shape
Straight Adductor Shape
REAR ONLY Adduction Area
FRONT ONLY Adduction Area

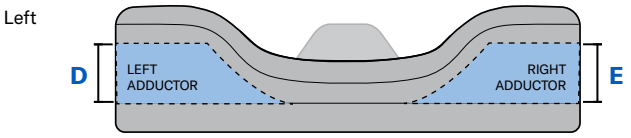

Rear view

MSRP HR Medium $47.00 | **Crosslink Firm** $47.00

A.

D	Left adductor height	E	Right adductor height
	D = ½" (CD-LEFT-ADD-0.5)		E = ½" (CD-RIGHT-ADD-0.5)
	D = 1" (CD-LEFT-ADD-1.0)		E = 1" (CD-RIGHT-ADD-1.0)
	D = 1 ½" (Standard) (CD-LEFT-ADD-1.5)		E = 1 ½" (Standard) (CD-RIGHT-ADD-1.5)
	D = 2" (CD-LEFT-ADD-2.0)		E = 2" (CD-RIGHT-ADD-2.0)
	D = 2 ½" (CD-LEFT-ADD-2.5)		E = 2 ½" (CD-RIGHT-ADD-2.5)
	D = Other_____ (CD-LEFT-ADD-OTHER)		E = Other_____ (CD-RIGHT-ADD-OTHER)

B.

	Left adductor style		Right adductor style
	Tapered adductor, HR Medium (CD-LEFT-ADD-TAPERED)		Tapered adductor, HR Medium (CD-RIGHT-ADD-TAPERED)
	Straight adductor, HR Medium (CD-LEFT-ADD-STRAIGHT)		Straight adductor, HR Medium (CD-RIGHT-ADD-STRAIGHT)
	Rear only straight adductor, HR Medium (CD-LEFT-ADD-REAR-ONLY)		Rear only straight adductor, HR Medium (CD-RIGHT-ADD-REAR-ONLY)
	Front only straight adductor, HR Medium (CD-LEFT-ADD-FRONT-ONLY)		Front only straight adductor, HR Medium (CD-RIGHT-ADD-FRONT-ONLY)
	Tapered adductor, Crosslink Firm (CD-LEFT-ADD-TAPERED-FIRM)		Tapered adductor, Crosslink Firm (CD-RIGHT-ADD-TAPERED-FIRM)
	Straight adductor, Crosslink Firm (CD-LEFT-ADD-STRAIGHT-FIRM)		Straight adductor, Crosslink Firm (CD-RIGHT-ADD-STRAIGHT-FIRM)
	Rear only straight adductor, Crosslink Firm (CD-LEFT-ADD-REAR-ONLY-FIRM)		Rear only straight adductor, Crosslink Firm (CD-RIGHT-ADD-REAR-ONLY-FIRM)
	Front only straight adductor, Crosslink Firm (CD-LEFT-ADD-FRONT-ONLY-FIRM)		Front only straight adductor, Crosslink Firm (CD-RIGHT-ADD-FRONT-ONLY-FIRM)

C.


	No adductor		No adductor
	None (CD-LEFT-ADD-NONE)		None (CD-RIGHT-ADD-NONE)

5.2 Abduction

MSRP HR Medium $47.00 | **Crosslink Firm** $47.00 each

INSTRUCTIONS: Select an abductor height and an abductor material.
NOTE: Custom abductor requests should be noted in the "Additional information" section 7.1.

Abductor height and material




Front view

	None (CD-ABD-NONE)		F = ½", Crosslink Firm (CD-ABD-HEIGHT-0.5-FIRM)
	F = ½", HR Medium (CD-ABD-HEIGHT-0.5)		F = 1", Crosslink Firm (CD-ABD-HEIGHT-1.0-FIRM)
	F = 1", HR Medium (CD-ABD-HEIGHT-1.0)		F = 1 ½", Crosslink Firm (CD-ABD-HEIGHT-1.5-FIRM)
	F = 1 ½", HR Medium (CD-ABD-HEIGHT-1.5)		F = 2", Crosslink Firm (CD-ABD-HEIGHT-2.0-FIRM)
	F = 2", HR Medium (CD-ABD-HEIGHT-2.0)		F = 2 ½", Crosslink Firm (CD-ABD-HEIGHT-2.5-FIRM)
	F = 2 ½", HR Medium (CD-ABD-HEIGHT-2.5)		F = Other, Crosslink Firm _____ (CD-ABD-HEIGHT-OTHER-FIRM)
	F = Other, HR Medium _____ (CD-ABD-HEIGHT-OTHER)		

5.3 Coccyx cutout

MSRP $47.00

NOTE: Coccyx cutout will be centered and cut in the lower layer of foam. If gel insert is selected, additional mid layer is required. **Cannot be paired with ROHO air insert. Cannot be paired with a recess in section 5.4.** Custom cutout requests should be noted in the "Additional information" section 7.1.

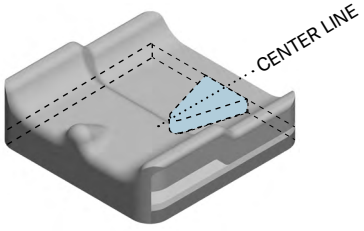

	Coccyx cutout (CD-COCCYX-CUT)

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

5.4 Recess
MSRP $255.00


NOTE: If a recess is selected, the mid layer foam thickness in section 4.3 must match the TOTAL amount of modifications selected in 2.1 and 5.2. **Cannot be paired with ROHO air insert or coccyx cutout.**

Rear quadrant recess



Front


L	Left side
	1/4" H (CD-IR-LEFT-REAR-0.25)
	1/2" H (CD-IR-LEFT-REAR-0.5)
	3/4" H (CD-IR-LEFT-REAR-0.75)
	1" H (CD-IR-LEFT-REAR-1.0)
	1 1/4" H (CD-IR-LEFT-REAR-1.25)
	Other _____ (CD-IR-LEFT-REAR-OTHER)



Front

R	Right side
	1/4" H (CD-IR-RIGHT-REAR-0.25)
	1/2" H (CD-IR-RIGHT-REAR-0.5)
	3/4" H (CD-IR-RIGHT-REAR-0.75)
	1" H (CD-IR-RIGHT-REAR-1.0)
	1 1/4" H (CD-IR-RIGHT-REAR-1.25)
	Other _____ (CD-IR-RIGHT-REAR-OTHER)

Full length recess



Front


L	Left side
	1/4" H (CD-IR-LEFT-FULL-0.25)
	1/2" H (CD-IR-LEFT-FULL-0.5)
	3/4" H (CD-IR-LEFT-FULL-0.75)
	1" H (CD-IR-LEFT-FULL-1.0)
	1 1/4" H (CD-IR-LEFT-FULL-1.25)
	Other _____ (CD-IR-LEFT-FULL-OTHER)



Front

R	Right side
	1/4" H (CD-IR-RIGHT-FULL-0.25)
	1/2" H (CD-IR-RIGHT-FULL-0.5)
	3/4" H (CD-IR-RIGHT-FULL-0.75)
	1" H (CD-IR-RIGHT-FULL-1.0)
	1 1/4" H (CD-IR-RIGHT-FULL-1.25)
	Other _____ (CD-IR-RIGHT-FULL-OTHER)


5.5 Hamstring relief
MSRP $57.00



Slide view
(Shown with an anti-thrust)

NOTE: Choose one hamstring relief option. Left or right side relief will be half the width of the cushion. Custom requests should be noted in "Additional information" section 7.1.


Full width relief



Front

G
G = 1" D (CD-HAM-RELIEF-1)
G = 2" D (CD-HAM-RELIEF-2)
G = Other _____ (CD-HAM-RELIEF-OTHER)


Left side relief



Front

G
G = 1" D (CD-LEFT-HAM-RELIEF-1)
G = 2" D (CD-LEFT-HAM-RELIEF-2)
G = Other _____ (CD-LEFT-HAM-RELIEF-OTHER)

Right side relief

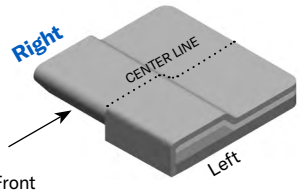


Front

G
G = 1" D (CD-RIGHT-HAM-RELIEF-1)
G = 2" D (CD-RIGHT-HAM-RELIEF-2)
G = Other _____ (CD-RIGHT-HAM-RELIEF-OTHER)

5.6 Growth notches
MSRP $57.00

NOTE: Growth notches may affect any adductors at the rear of the seat support. *Tip: An anti-thrust growth kit from section 2.2 subsection A can be used to adjust the seat well depth as well, if an anti-thrust feature is needed.*

Depth of notches

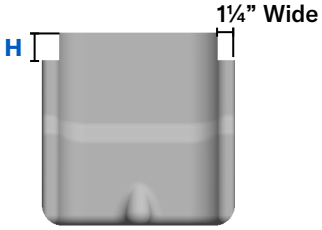

Top view

H
H = 1" D (CD-GROWTH-NOTCH-1)
H = 2" D (CD-GROWTH-NOTCH-2)
H = 3" D (CD-GROWTH-NOTCH-3)
H = Other_____ (CD-GROWTH-NOTCH-OTHER)

5.7 Rail cuts
MSRP $57.00

NOTE: Rail cuts will affect how much cushion is left along the sides of especially low-profile seat supports. **Cannot be paired with Removable Solid Seat Pan or ATI.**

Rail cut height



Front view

J
J = 1" Rail cut (CD-RAIL-CUT-1.0)
J = 1 ½" Rail cut (CD-RAIL-CUT-1.5)
J = 2" Rail cut (CD-RAIL-CUT-2.0)
J = Other _____ (CD-RAIL-CUT-OTHER)


"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

5.8 Leg length discrepancy

MSRP $167.00


NOTE: Offset discrepancy maintains foam abductor shape and removable abductor placement.

Standard leg length discrepancy

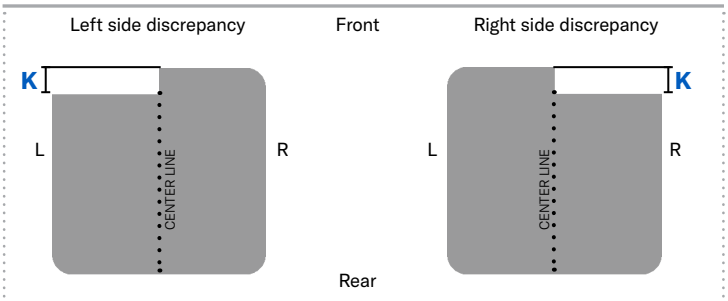

L	Depth removed from side			R
	(CD-LLD-DEPTH-L-0.5)	**K** = ½" D	(CD-LLD-DEPTH-R-0.5)	
	(CD-LLD-DEPTH-L-1.0)	**K** = 1" D	(CD-LLD-DEPTH-R-1.0)	
	(CD-LLD-DEPTH-L-1.5)	**K** = 1½" D	(CD-LLD-DEPTH-R-1.5)	
	(CD-LLD-DEPTH-L-2.0)	**K** = 2" D	(CD-LLD-DEPTH-R-2.0)	
	(CD-LLD-DEPTH-L-OTHER)	**K** = Other_____	(CD-LLD-DEPTH-R-OTHER)	

Offset leg length discrepancy

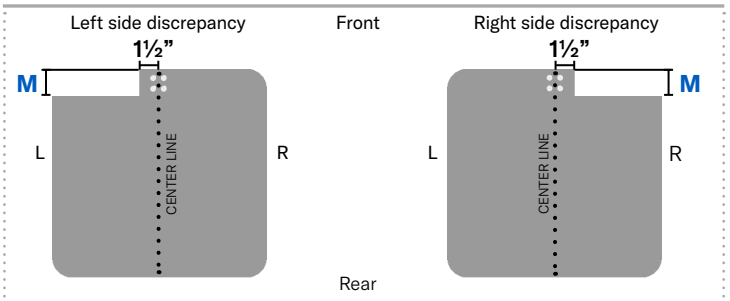

L	Depth removed from side			R
	(CD-LLD-O-DEPTH-L-0.5)	**M** = ½" D	(CD-LLD-O-DEPTH-R-0.5)	
	(CD-LLD-O-DEPTH-L-1.0)	**M** = 1" D	(CD-LLD-O-DEPTH-R-1.0)	
	(CD-LLD-O-DEPTH-L-1.5)	**M** = 1½" D	(CD-LLD-O-DEPTH-R-1.5)	
	(CD-LLD-O-DEPTH-L-2.0)	**M** = 2" D	(CD-LLD-O-DEPTH-R-2.0)	
	(CD-LLD-O-DEPTH-L-OTHER)	**M** = Other_____	(CD-LLD-O-DEPTH-R-OTHER)	

5.9 Platform

MSRP $828.00

NOTE: Accommodates 7/8" or 1" tubing. Comes with two different cross bars to accommodate various wheelchair frame types. Fits both folding and non-folding seat rails. Lateral pelvic/thigh support hardware can be easily attached. **Cannot be paired with rail cut.** Leg length discrepancy offset maintains centered removable abductor hardware attachment.

Removable solid seat pan




	Solid seat pan CD-RSSP-N-HARD)
	Solid seat pan w/standard leg discrepancy CD-RSSP-STND-HARD)
	Solid seat pan w/offset leg discrepancy CD-RSSP-OFF-LLD)

5.10 Insert

NOTE: Moldable ATI (Adjustable Technology Insert for Positioning) enables on-site customization to the contour of the seat support surface. **1/4" Crosslink is not recommended with the ATI. Cannot be paired with rail cuts.**

Moldable ATI

See cushion pricing on page 2




	Moldable ATI (CD-MOLDABLE-INSERT)

NOTE: **Cannot be paired with the round bottom in section 2.1.**

Rigid insert

MSRP $135.00



	Rigid insert glued (CD-RGD-INSERT-GLUED)
	Rigid insert not glued (CD-RGD-INSERT-UNGLUED)

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

6 Cover & accessories

6.1 Custom cover material options

MSRP Standard $0.00 | **w/GlideWear** $38.00

COMFORT-TEK®

A smooth, easily cleaned surface. The incontinence protection also aids in infection control.

OR

STRETCH-AIR®

Stretch-Air has comfortable stretch and heat dissipation.

GlideWear™
Shear reduction panel

Selected for shear reduction, micro-climate control and improved comfort. This fabric panel sits below the bony prominences for maximum skin protection.

COMFORT-TEK	
☐ **Standard** (CD-COMFORT-TEK)	☐ **WITH GlideWear** (CD-GW-COMFORT-TEK)

STRETCH-AIR	
☐ **Standard** (CD-STRETCH-AIR)	☐ **WITH GlideWear** (CD-GW-STRETCH-AIR)

6.2 Extra custom cover

MSRP Standard $135.00 | **w/GlideWear** $145.00

COMFORT-TEK	
☐ **Standard** (CD-X-COMFORT-TEK)	☐ **WITH GlideWear** (CD-GW-X-COMFORT-TEK)

STRETCH-AIR	
☐ **Standard** (CD-X-STRETCH-AIR)	☐ **WITH GlideWear** (CD-GW-X-STRETCH-AIR)

6.3 Incontinence liner

MSRP $0.00

NOTE: If a ROHO air insert is selected, Incontinence liner will have a small opening for the valve hose.

☐ Incontinence liner (CD-INCON-LINER)

6.4 Zippered pouch

MSRP $57.00


☐ Zippered pouch (CD-ZIP-POUCH)

6.5 Colored piping

MSRP $0.00

NOTE: If no color is selected, our standard silver reflective piping will be used.

☐ Red (CD-RED)	☐ Blue (CD-BLUE)
☐ Purple (CD-PURPLE)	☐ Green (CD-GREEN)
☐ Pink (CD-PINK)	☐ Remove (CD-REMOVE)
☐ Orange (CD-ORANGE)	

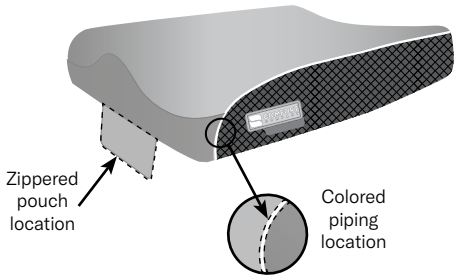

7 Additional information

7.1 Comments

INSTRUCTIONS: Please reference any section or subsection of the form when making any comments.

Section #	Page #	Comments

INSTRUCTIONS: If preferred, please sketch ideas in the spaces provided below.

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."